


EXO

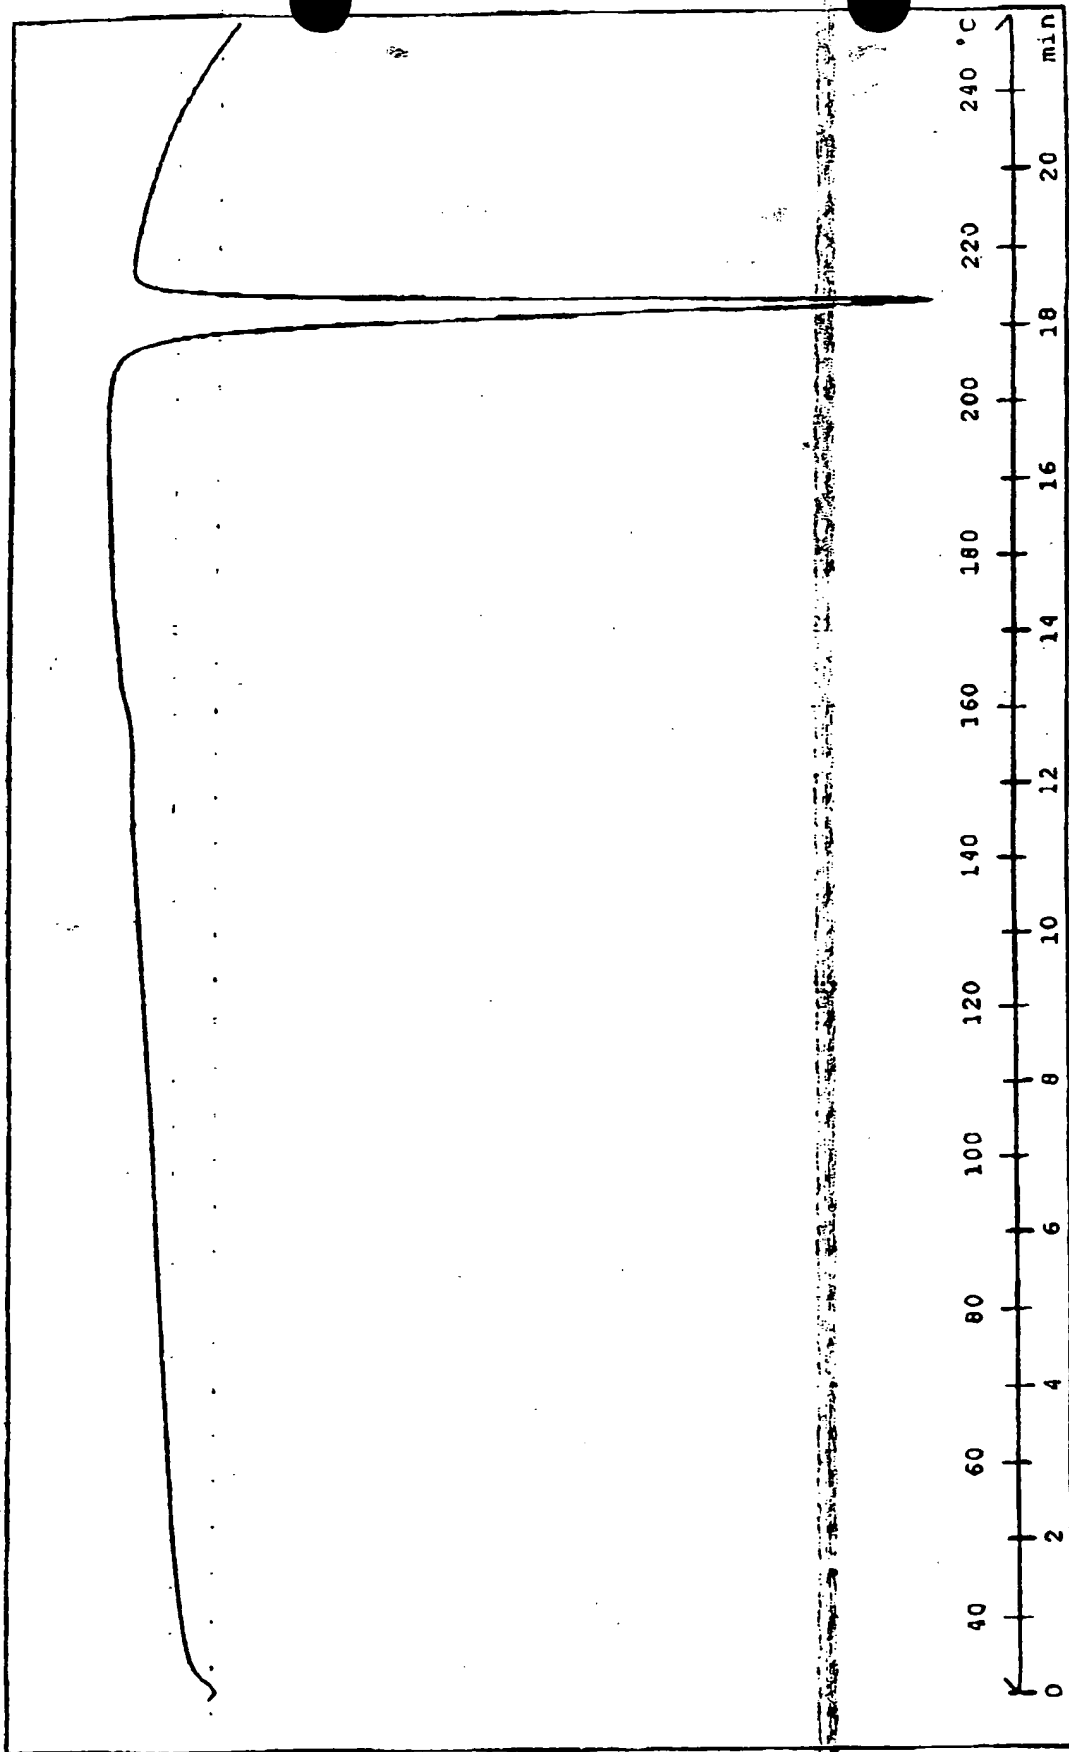

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR System

Figure 1

FOOT OF SHOOT


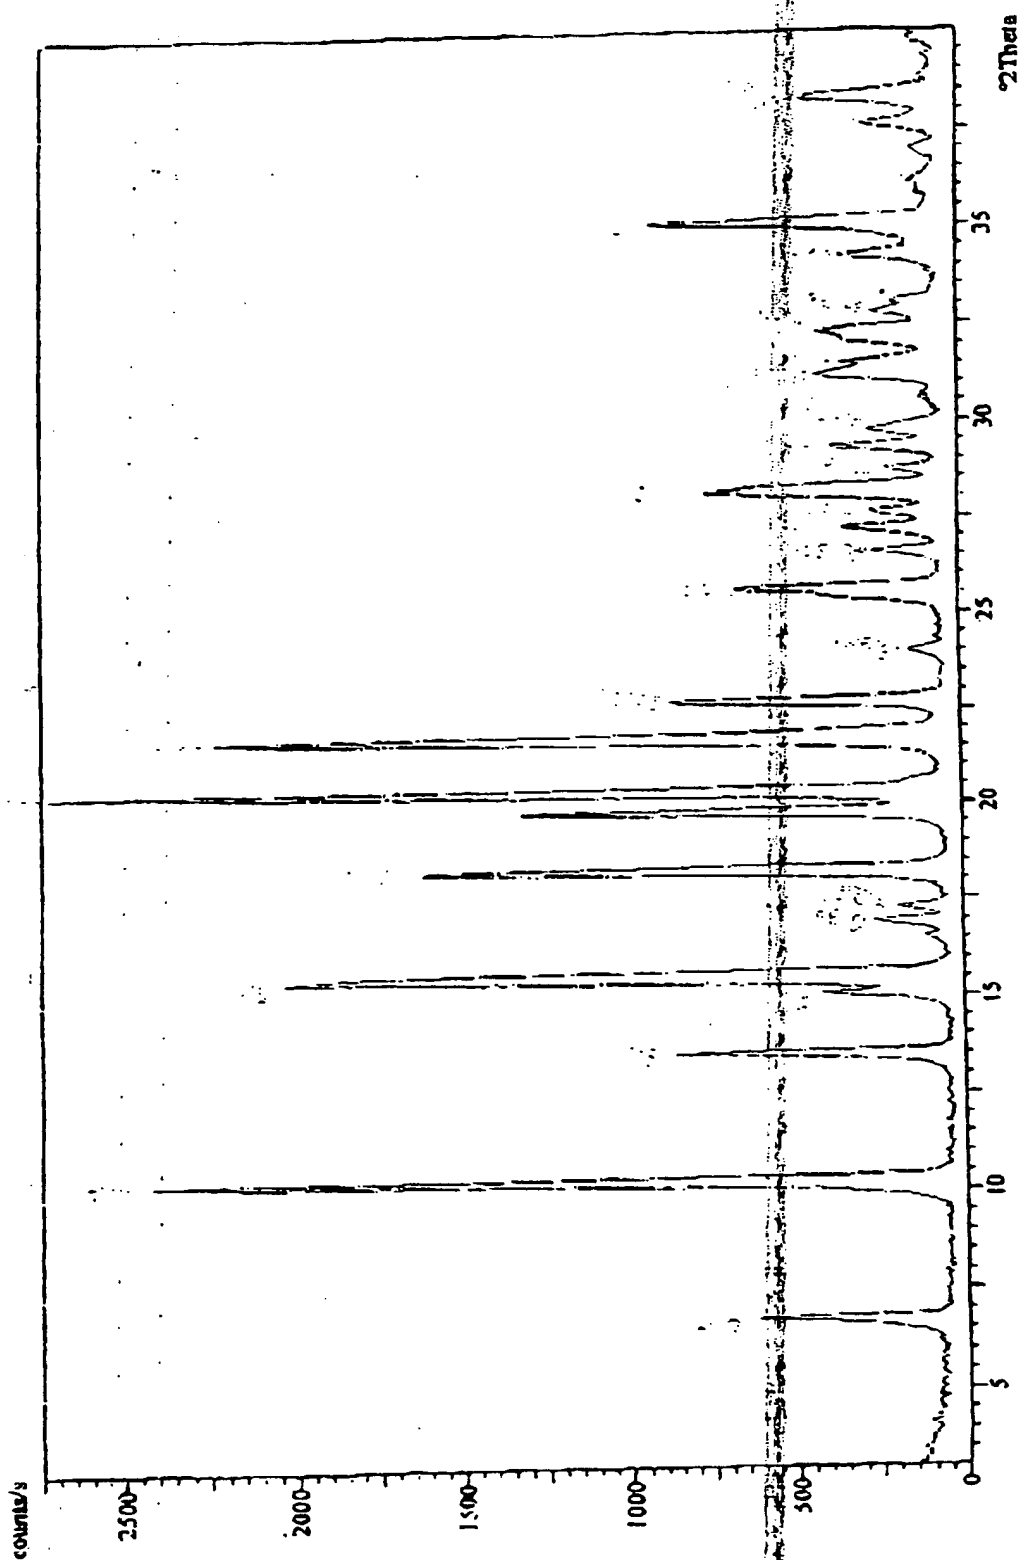


Figure 2

exo

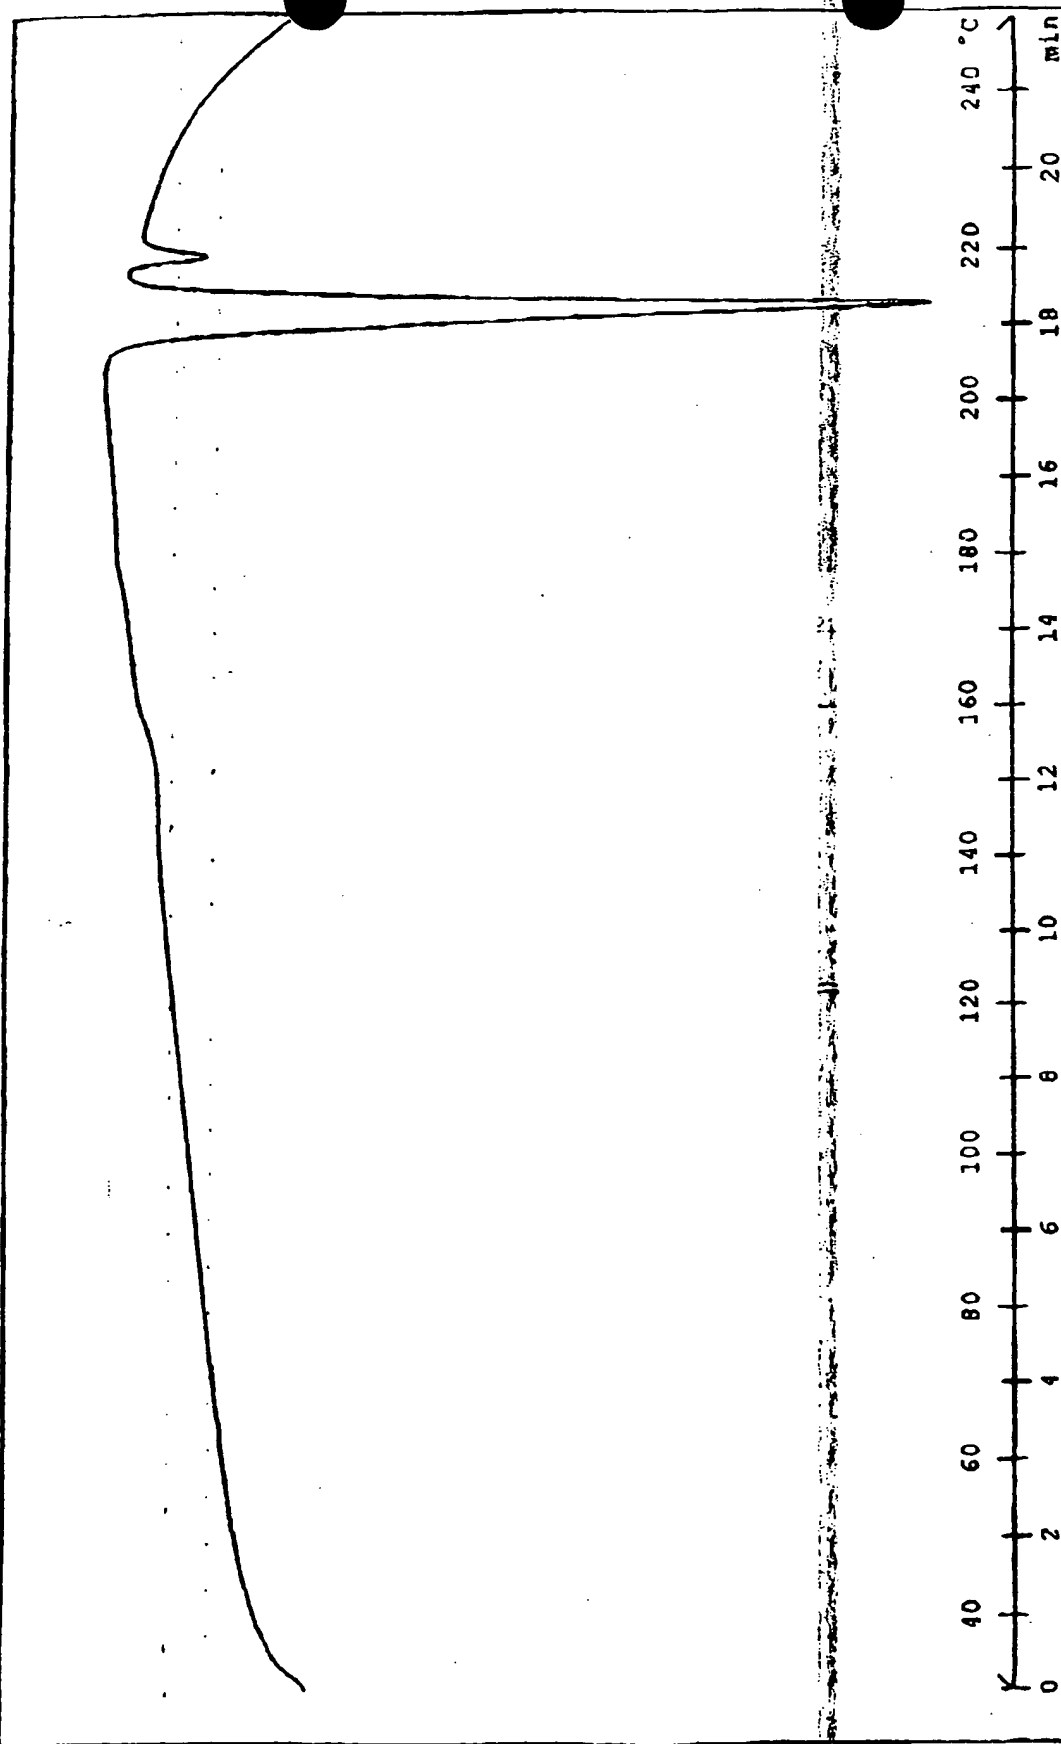

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR® System

Figure 3


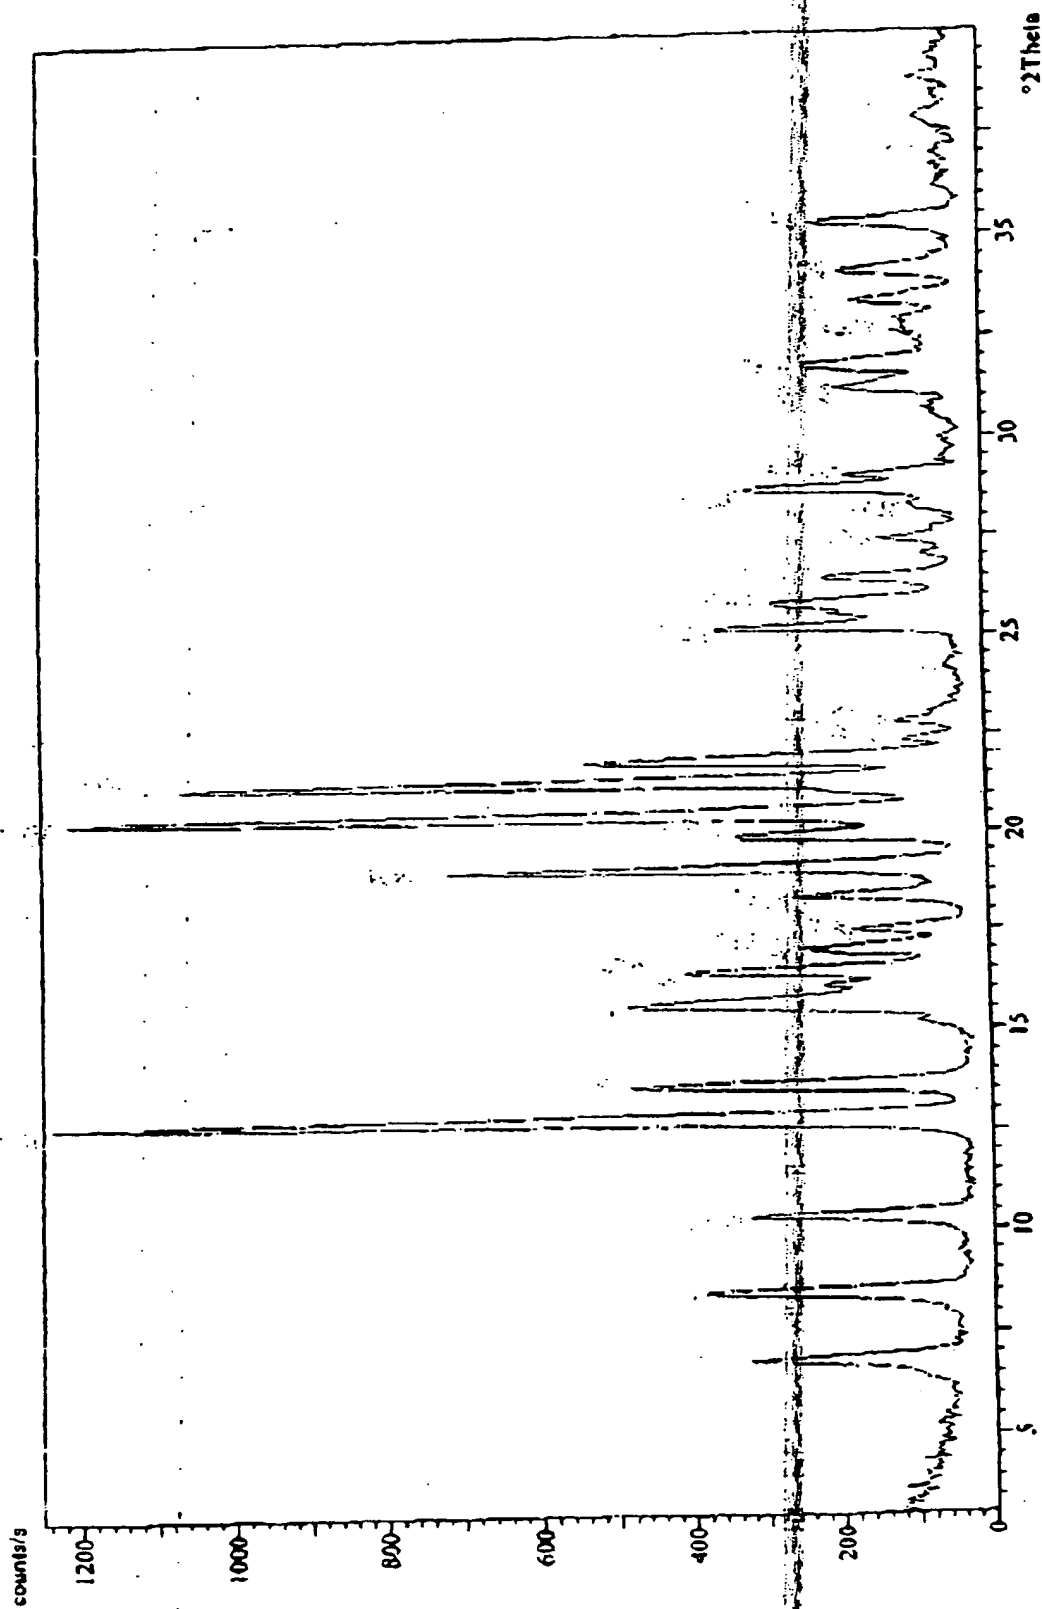


Figure 4

exo

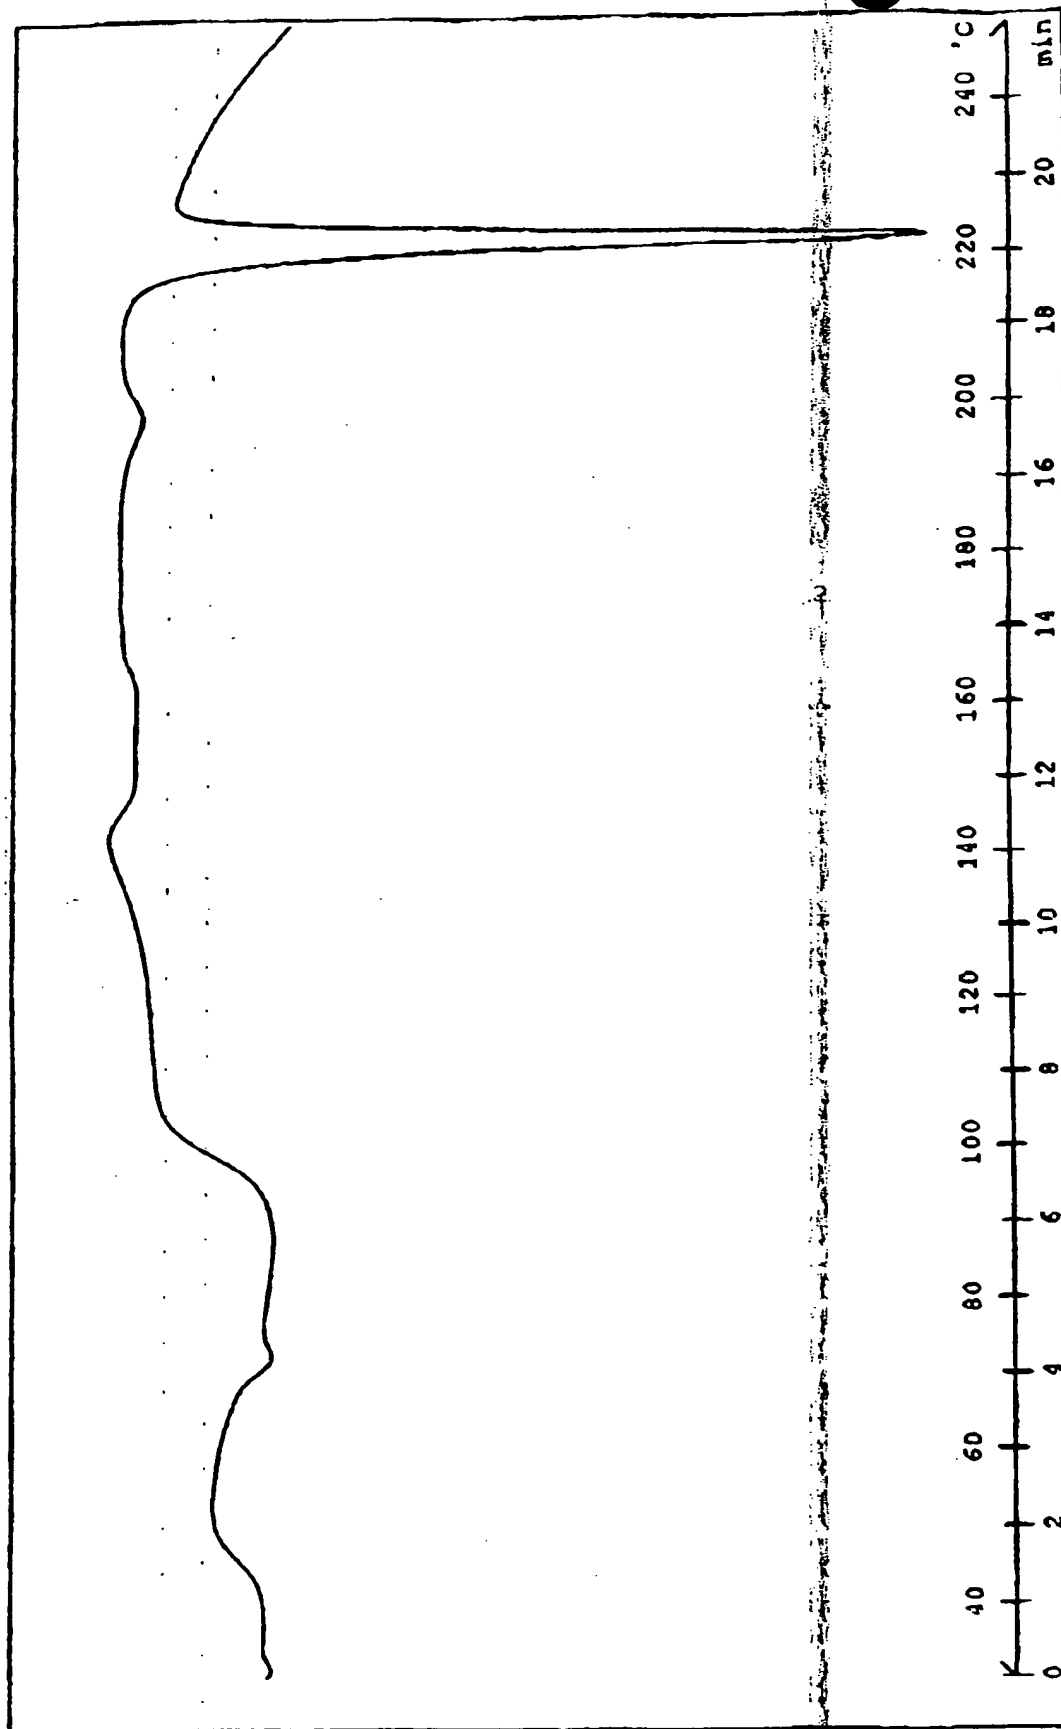

Physical R&D Teva: Shlomo

METTLER TOLEDO STAR® System

Figure 5

T06TOT OTS400T

TOTAL P.03


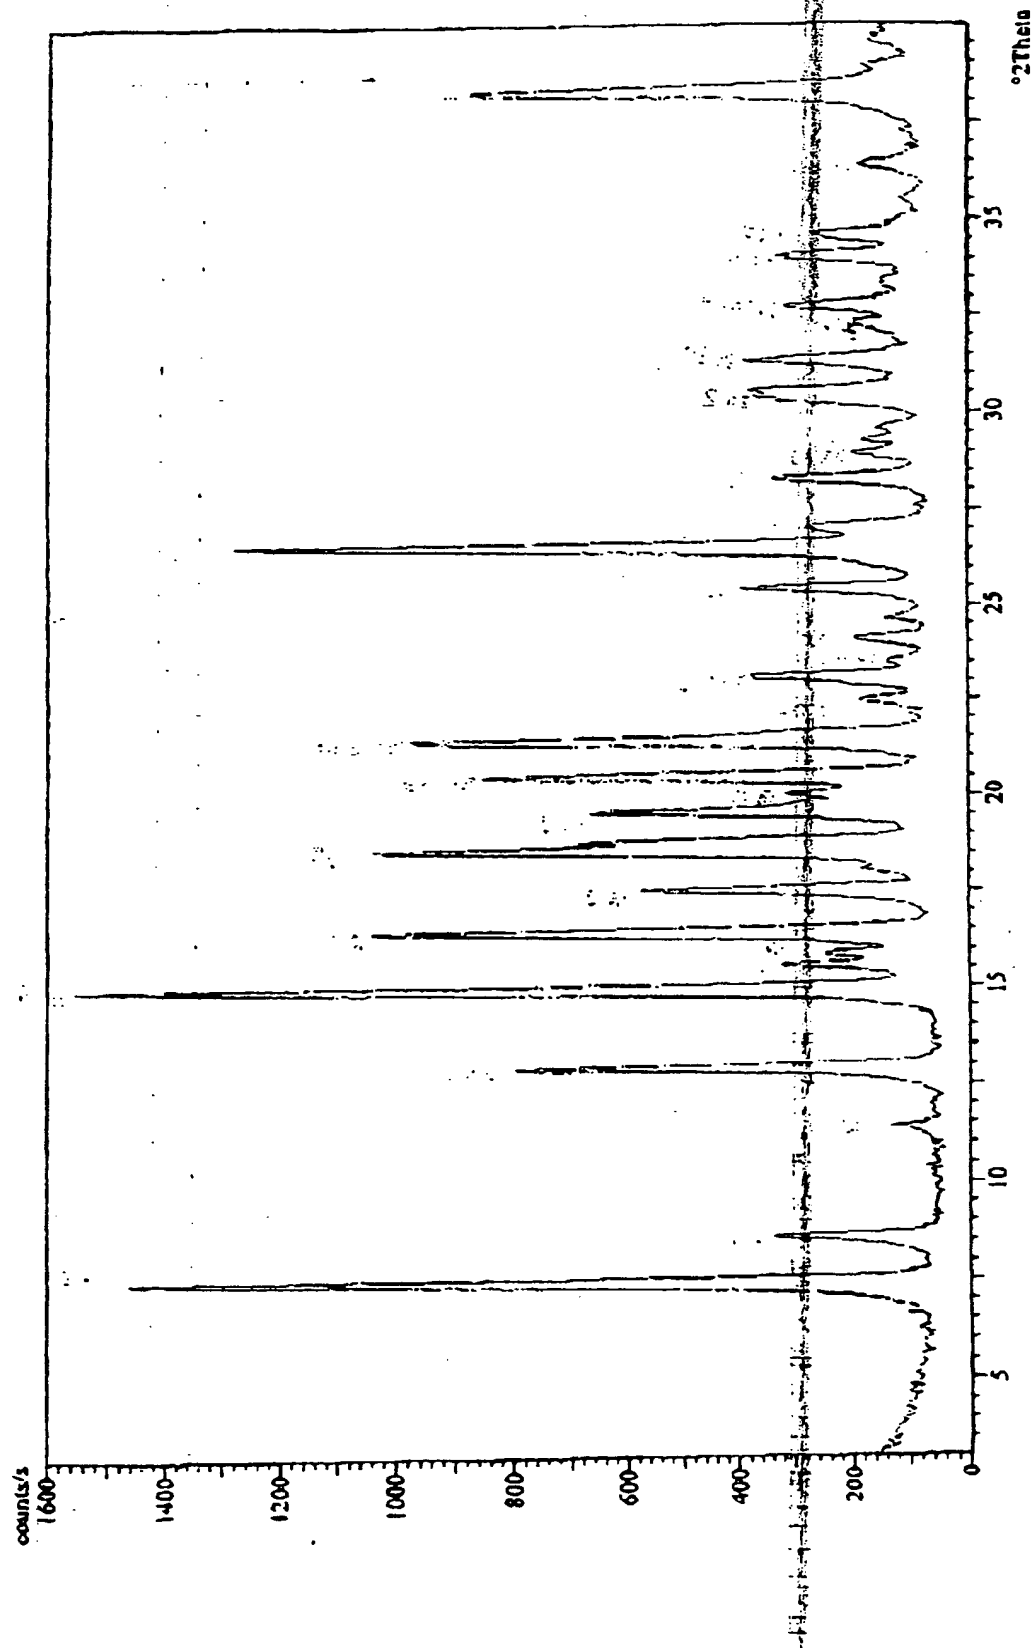


Figure 6

TOOT OF SHOOT

EXO

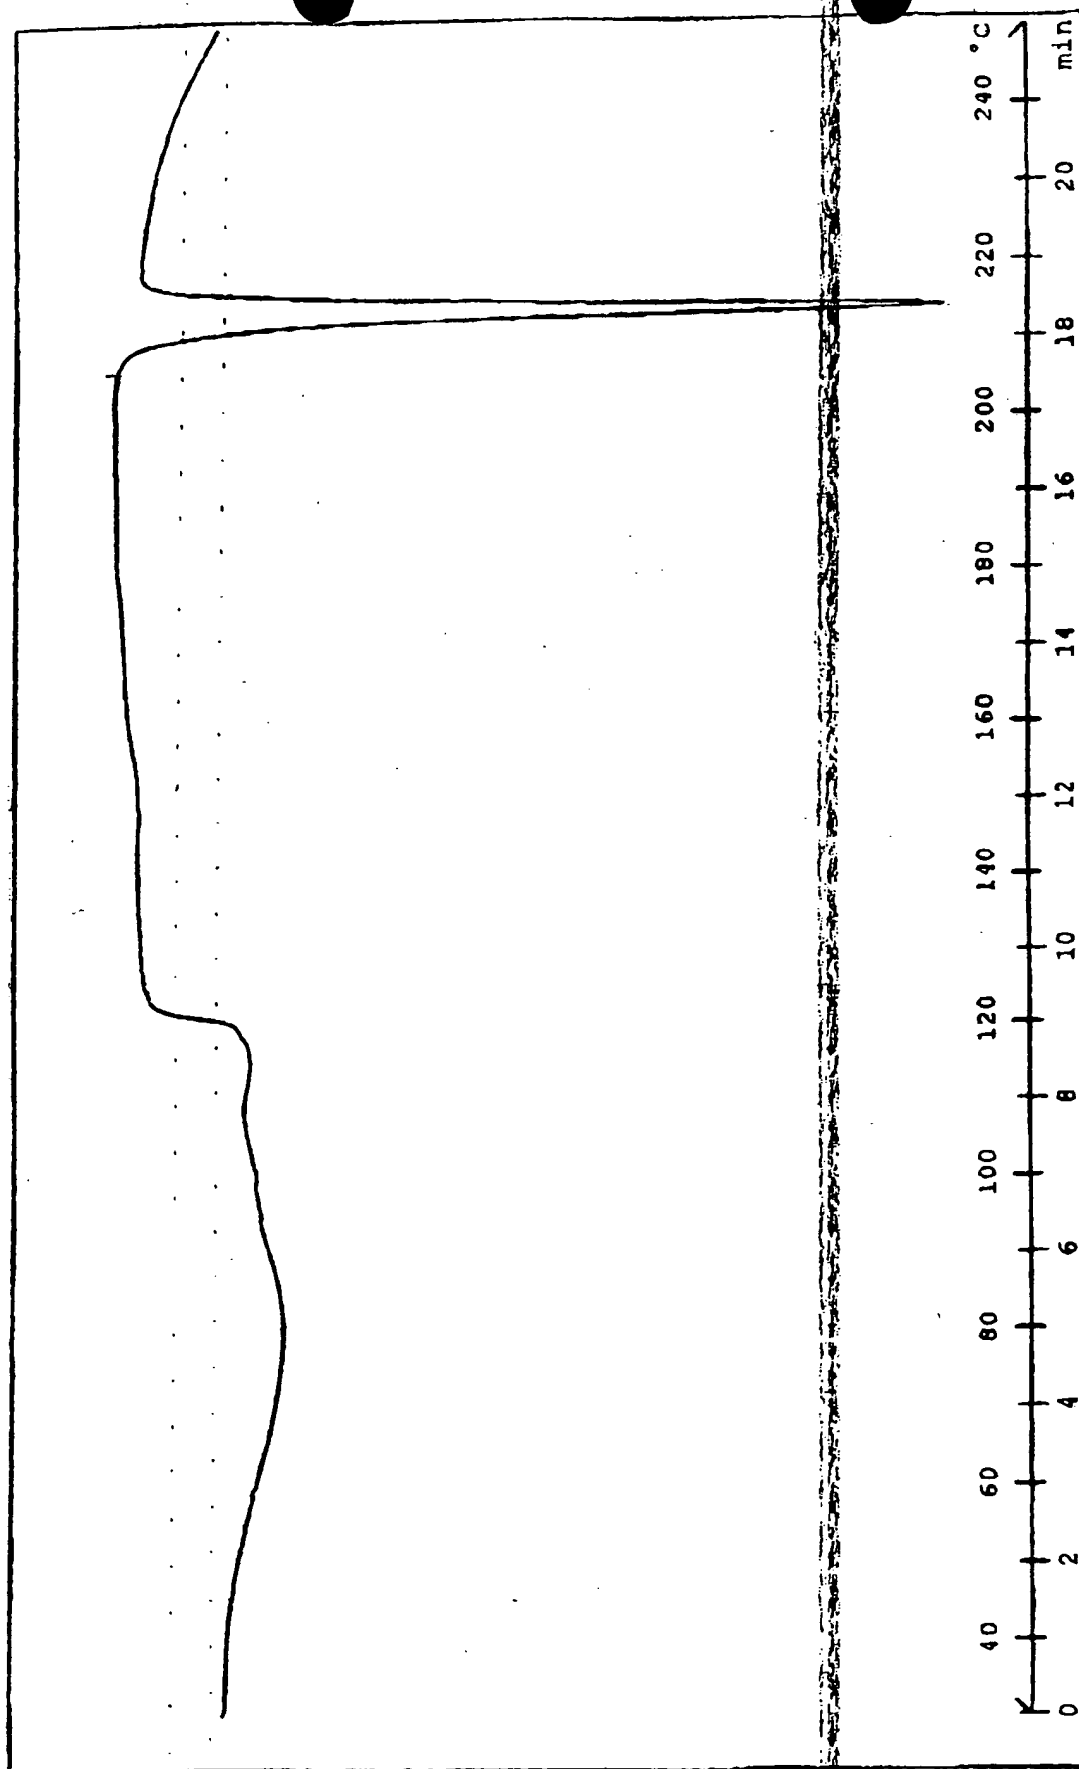

Physical R&D Teva: Shlomo

METTLE TOLEDO STAR® System

Figure 7

PRINT OF DRAWINGS
AS ORIGINALLY FILED

100 TOT OF 500T

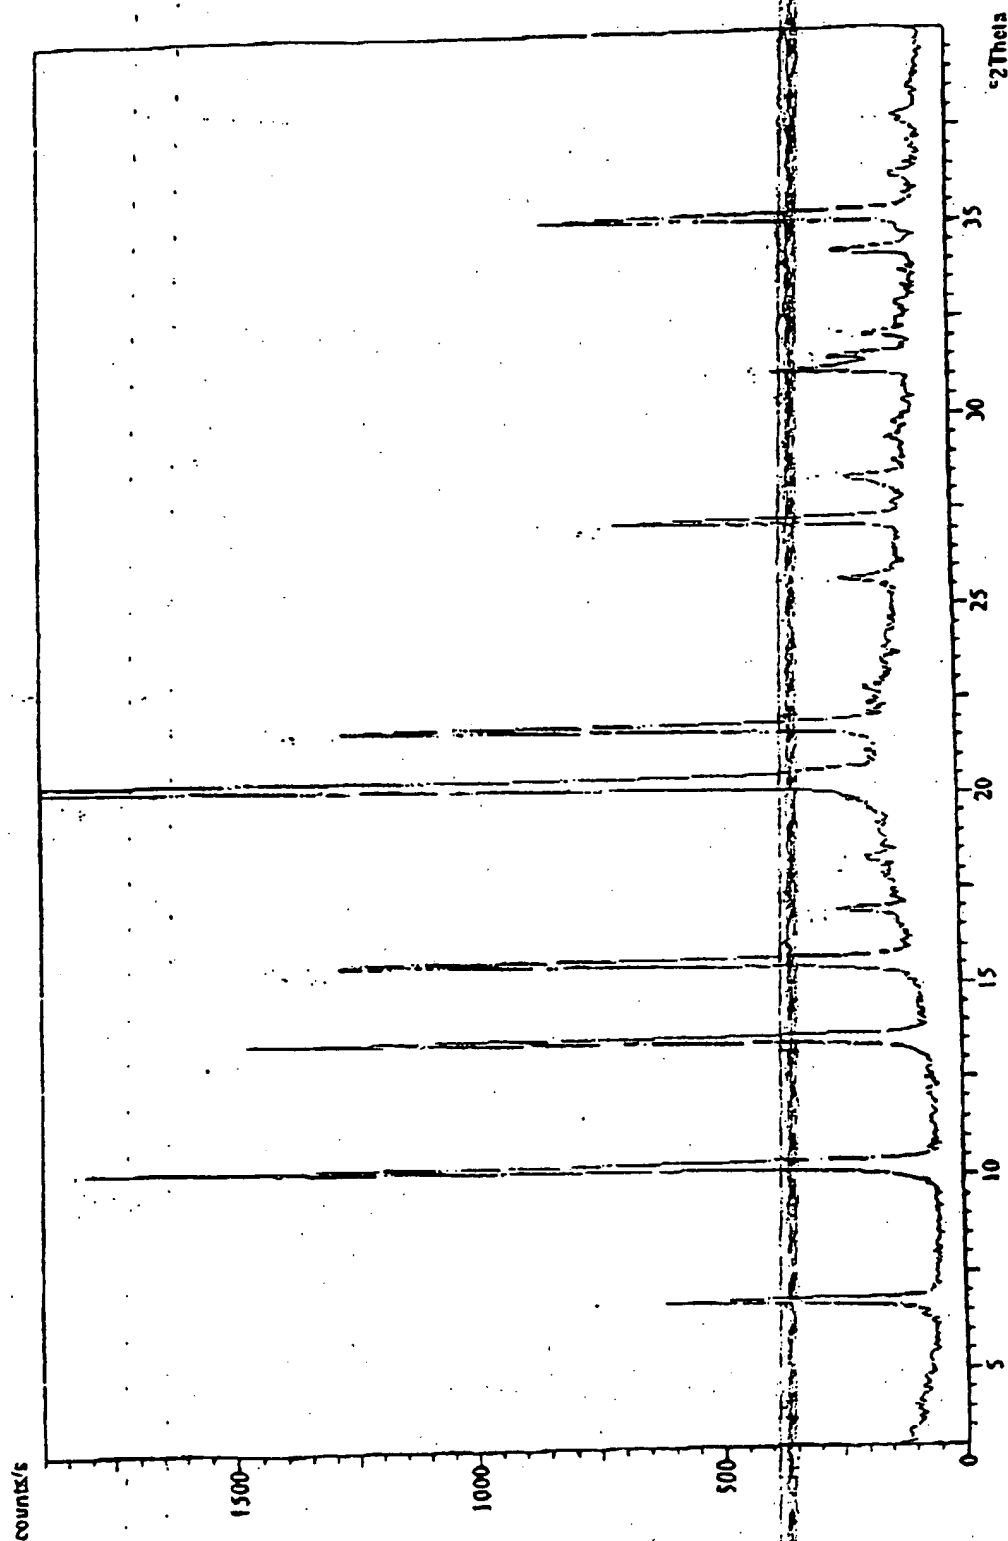


Figure 8

TOTAL CHARGE

File: VZL-07 SHQ, ID: VZL-07 SHQ.
Date: 02/01/01 13:16 Step: 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) C nt. Scan Rate: 3.00 Deg/min. TEVA

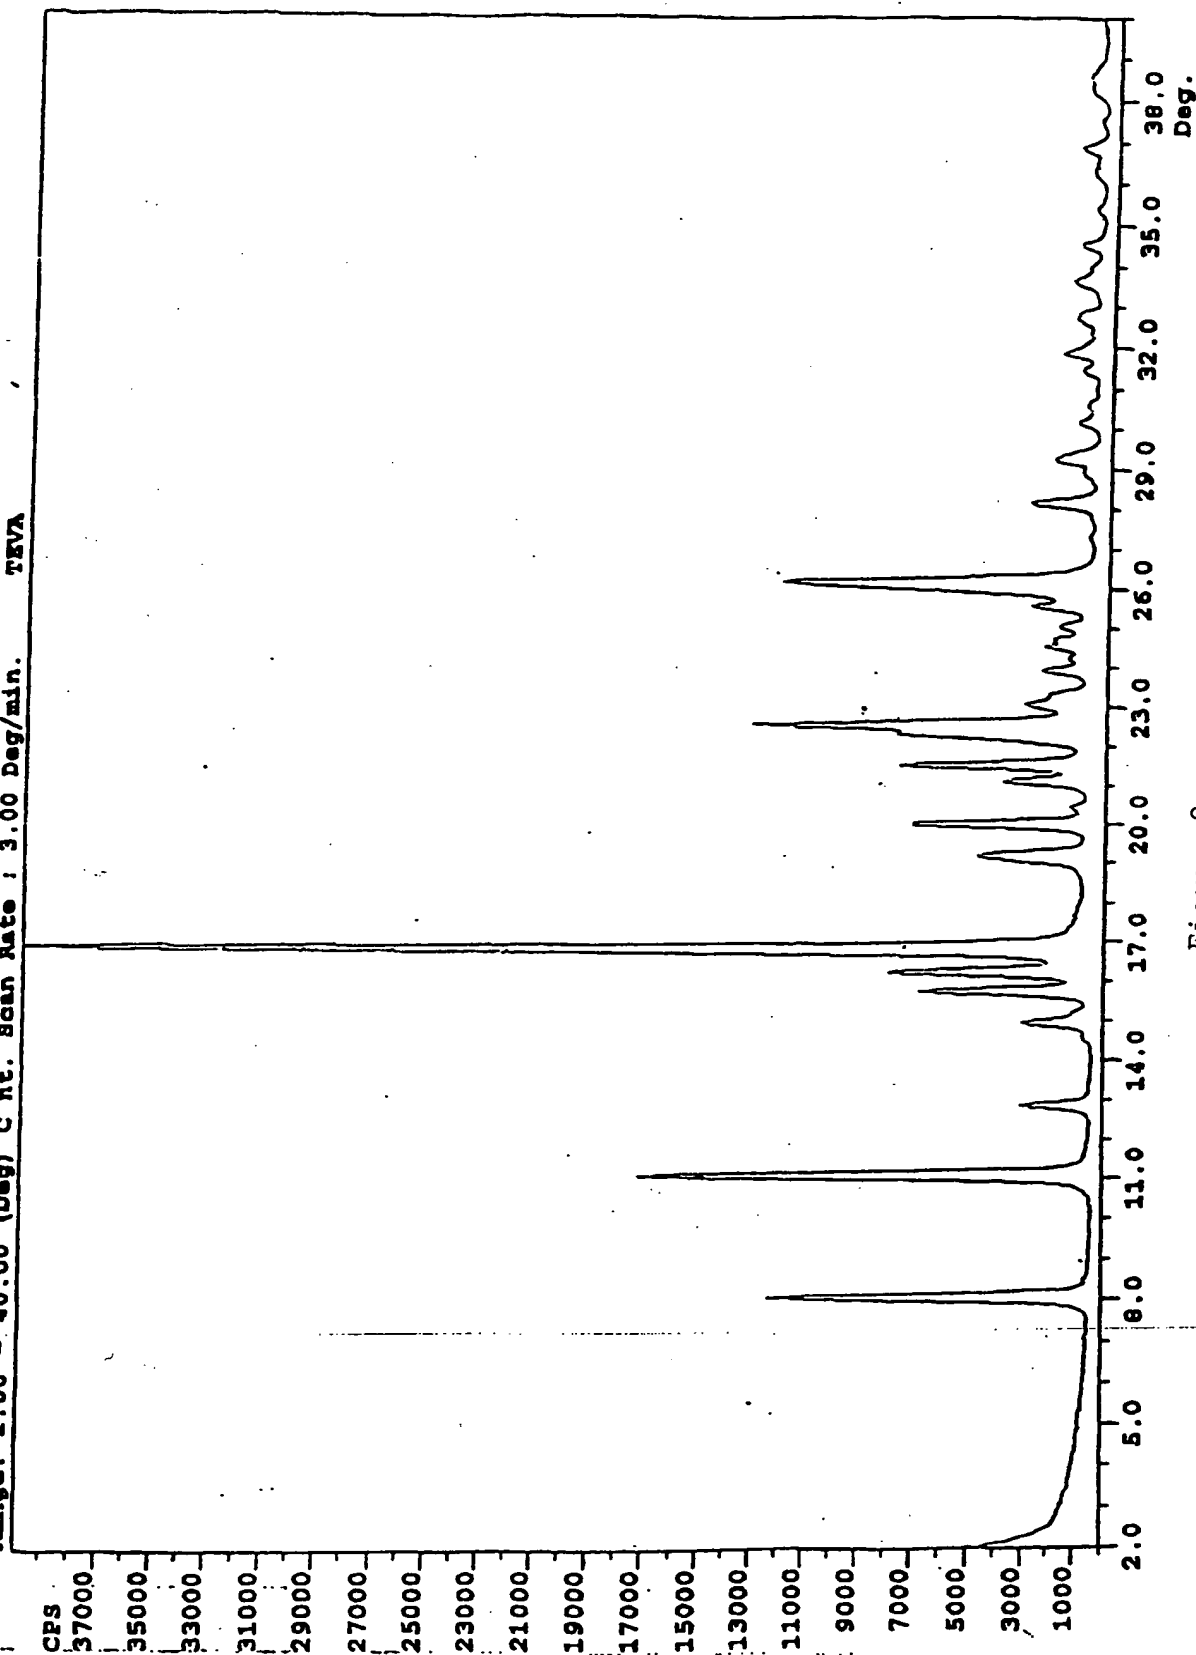


Figure 9

FIGURE 10

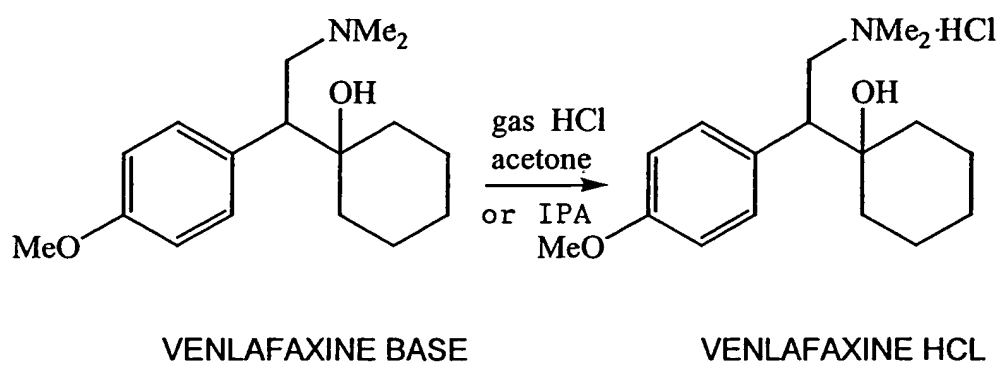


FIGURE 10